




METHOD AND SYSTEM FOR CONTROL OF A PATIENT'S BODY TEMPERATURE . . . HEAT EXCHANGE CATHETER Machold et al. Div. of 09/707,257


Docket No. RADME-65147

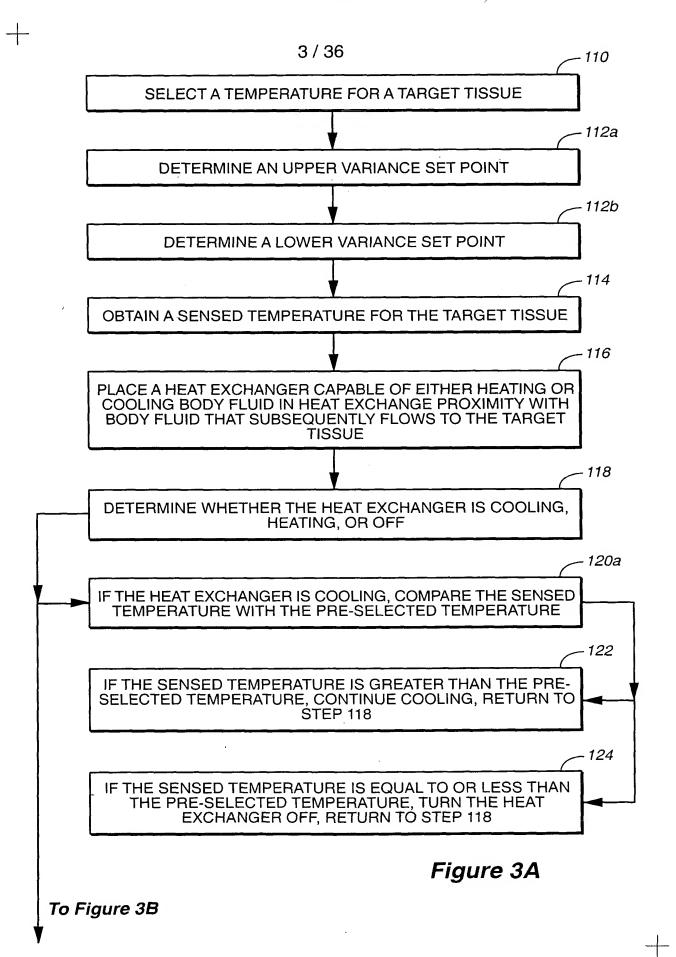


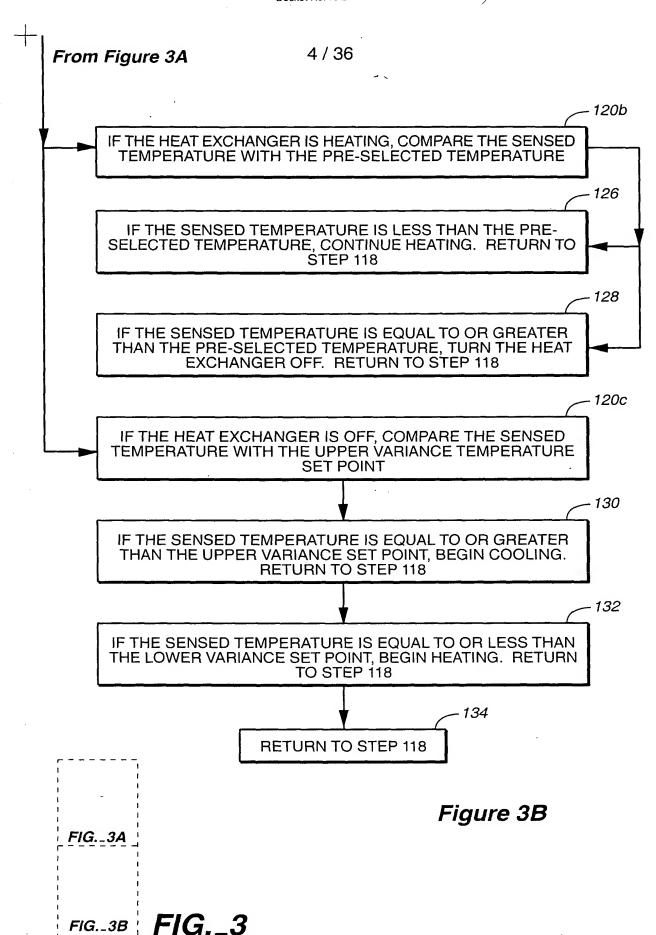


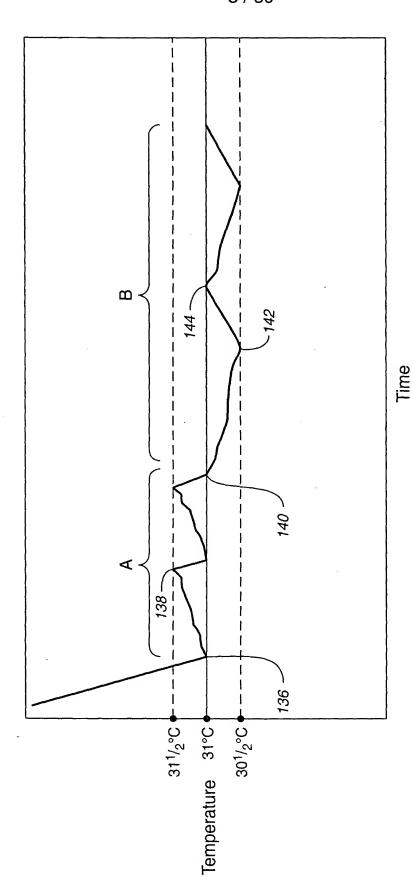


31°C = Pre-selected temperature 311/2°C = Upper variance set point 301/2°C = Lower variance set point

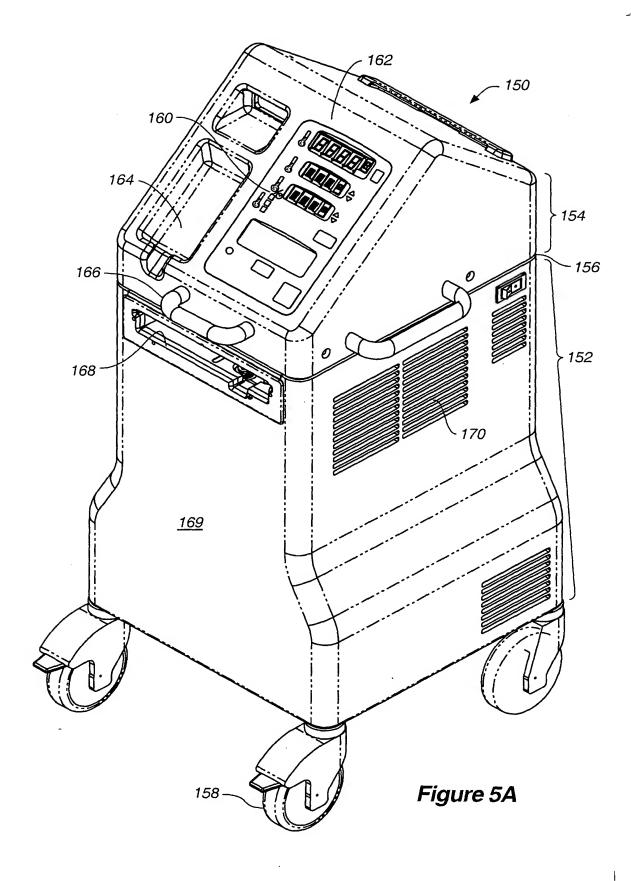


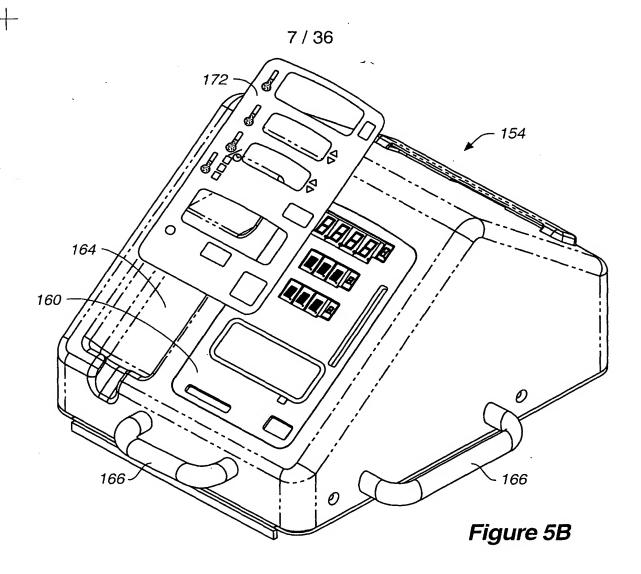

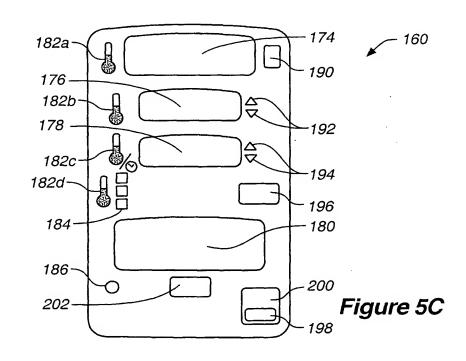


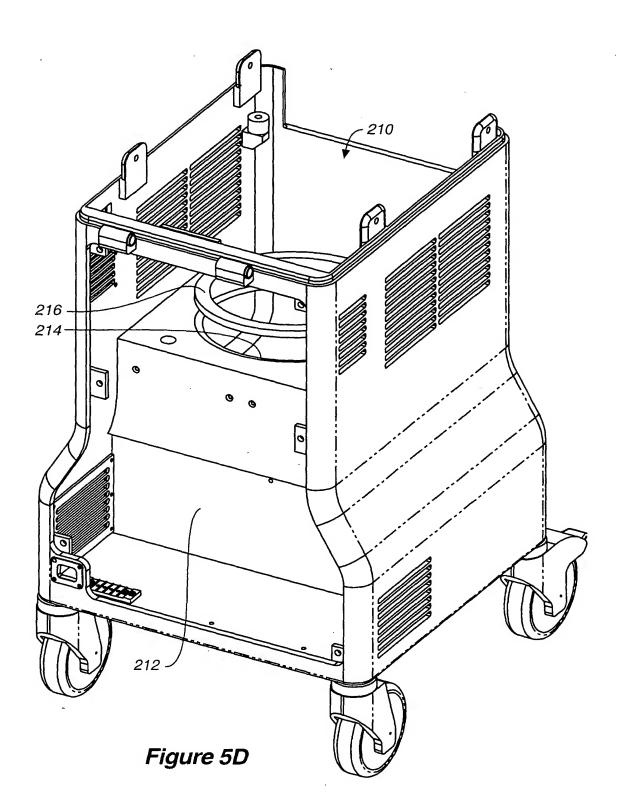


+

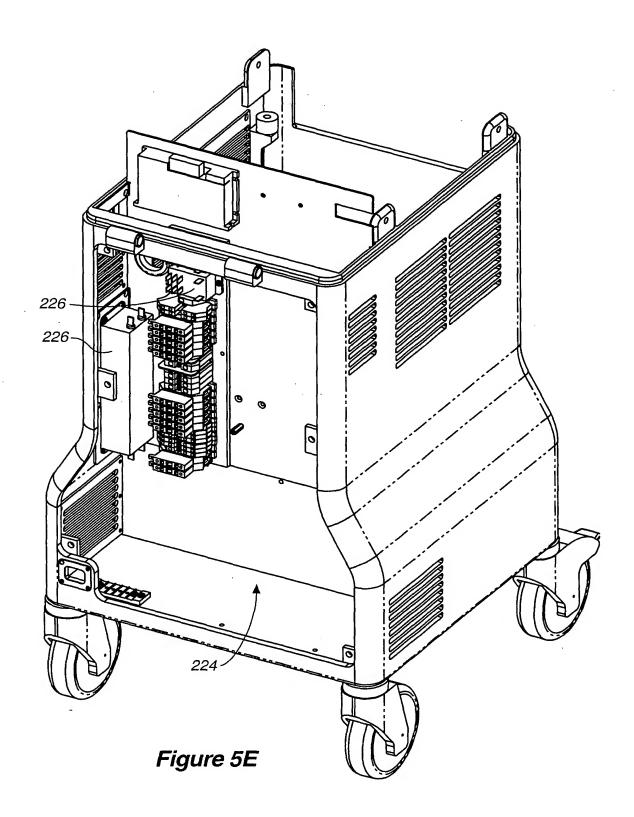



L

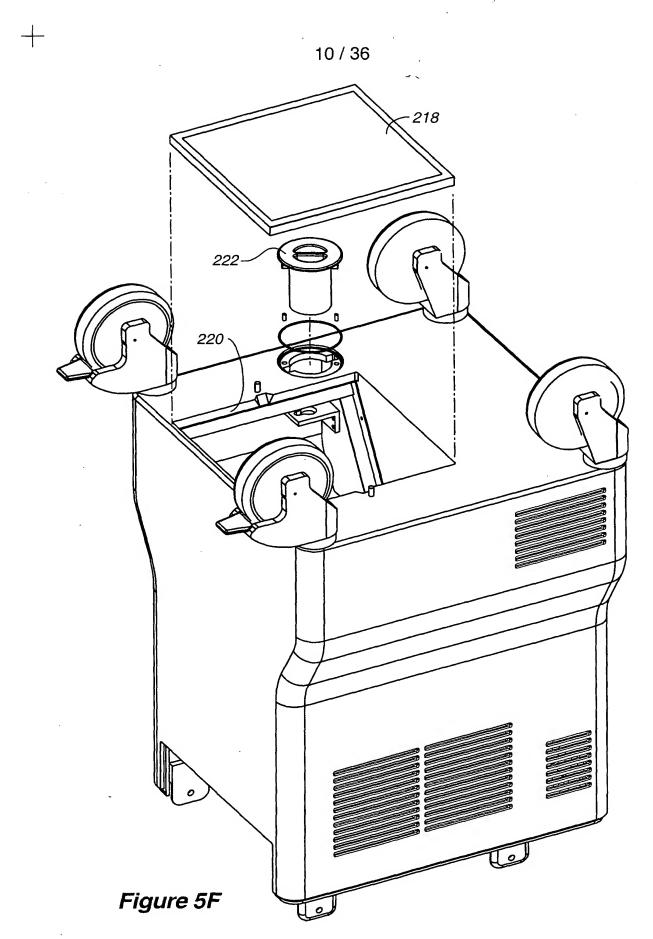



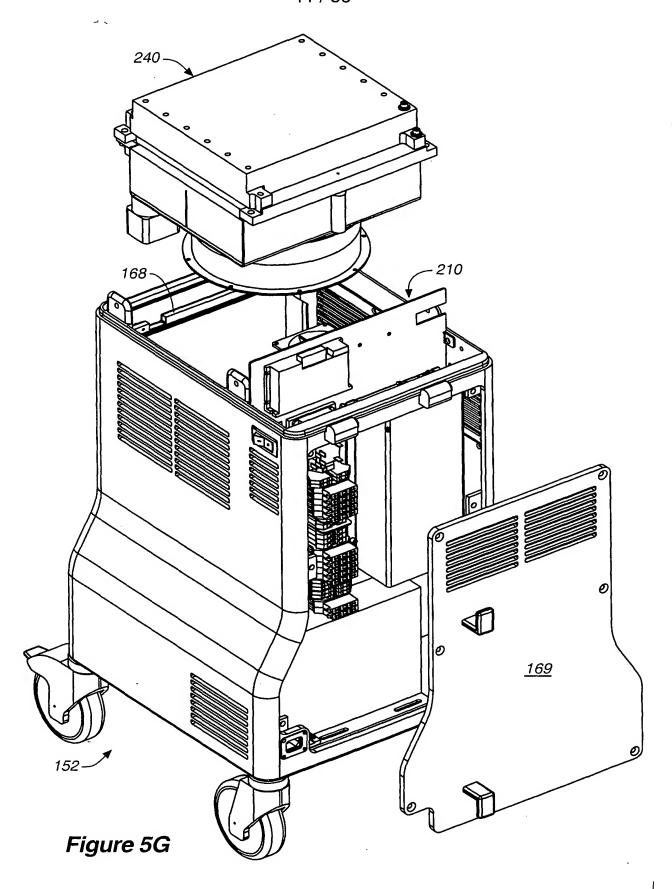

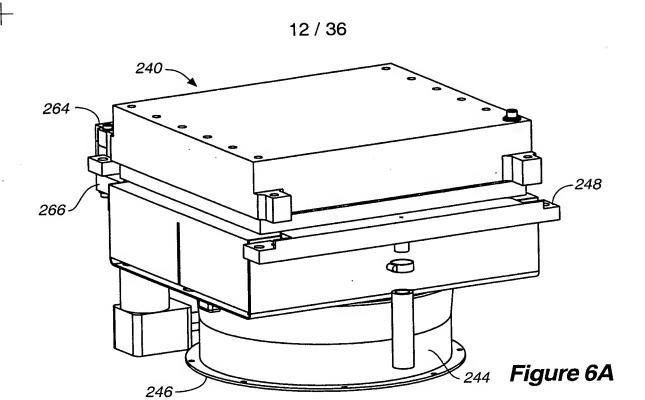

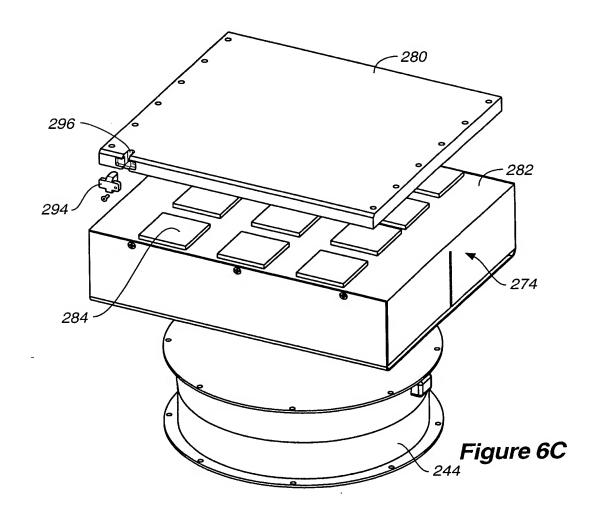

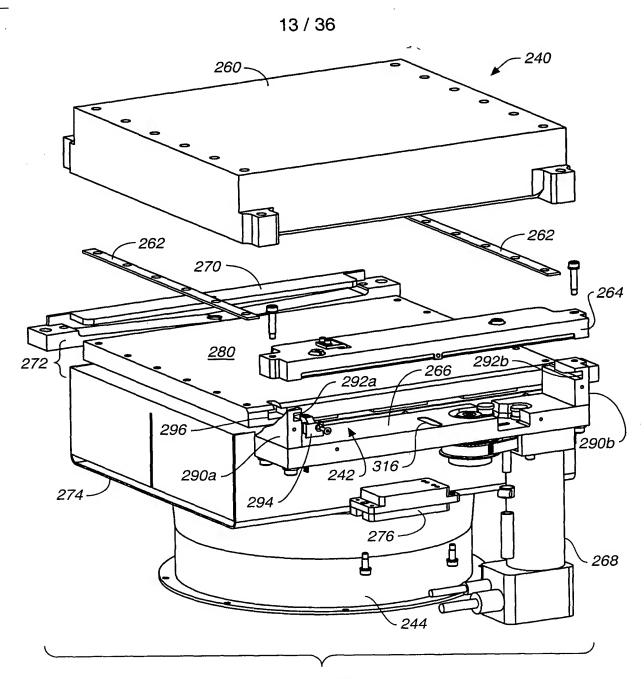
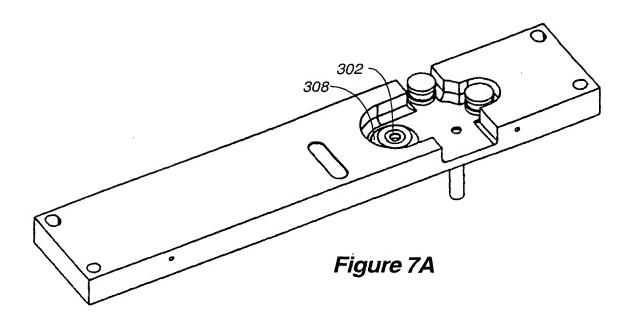


Figure 6B



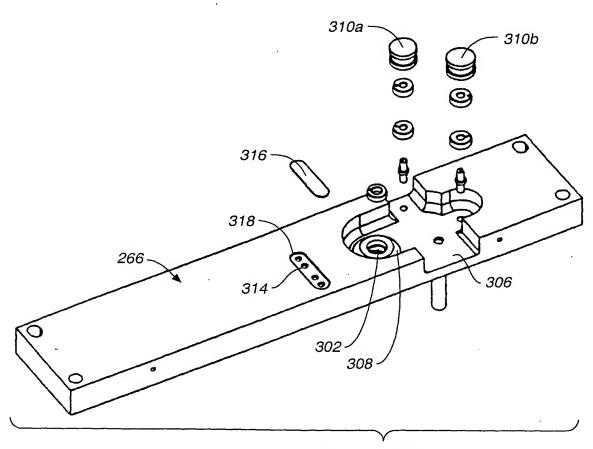
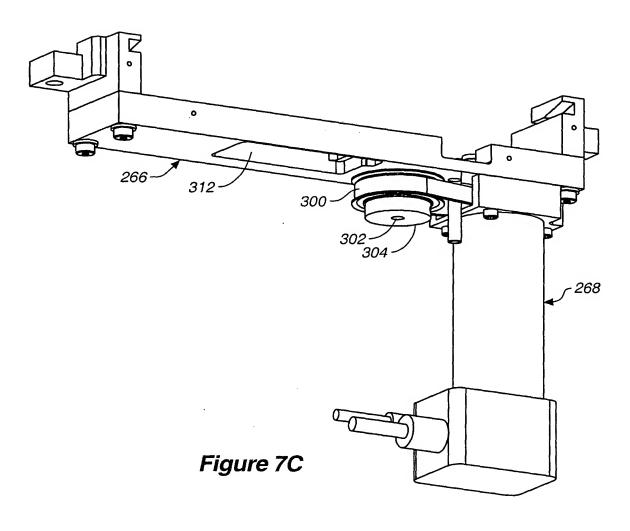


Figure 7B






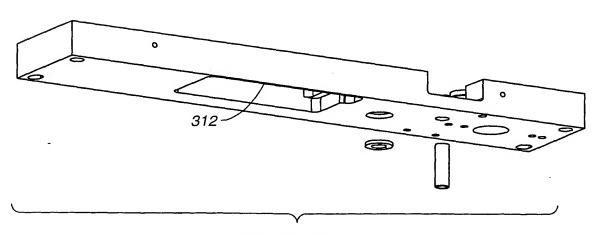



Figure 7D

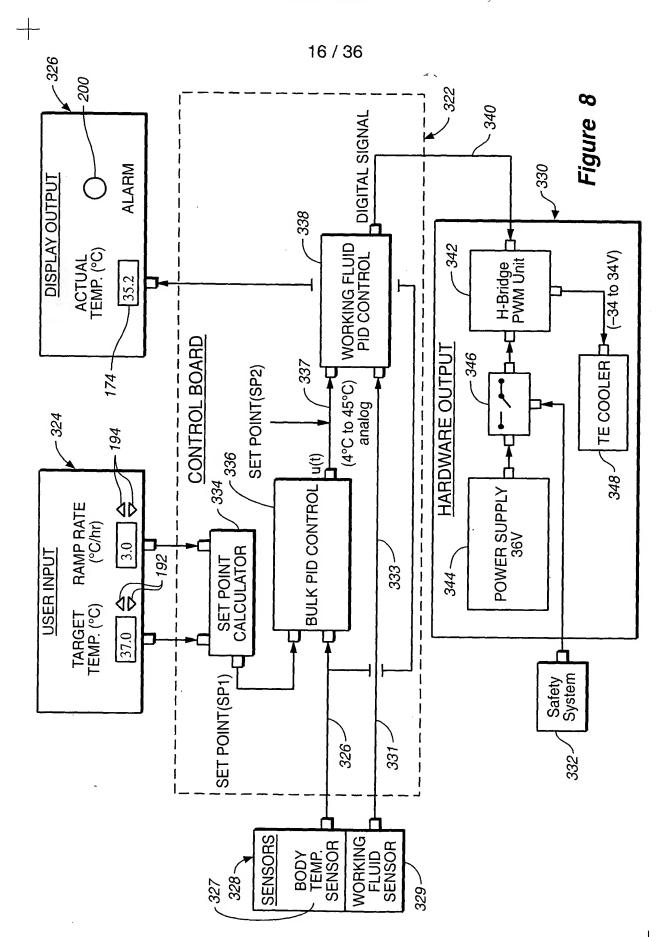


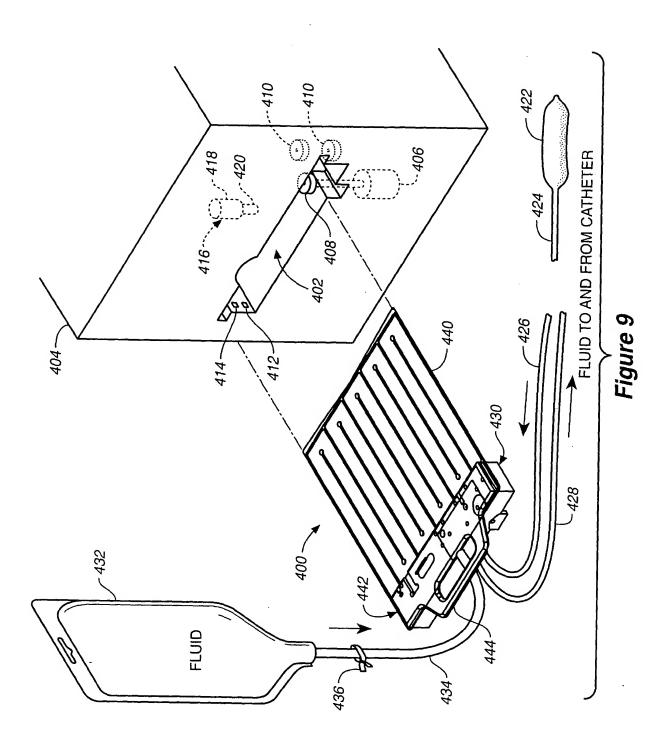



╀

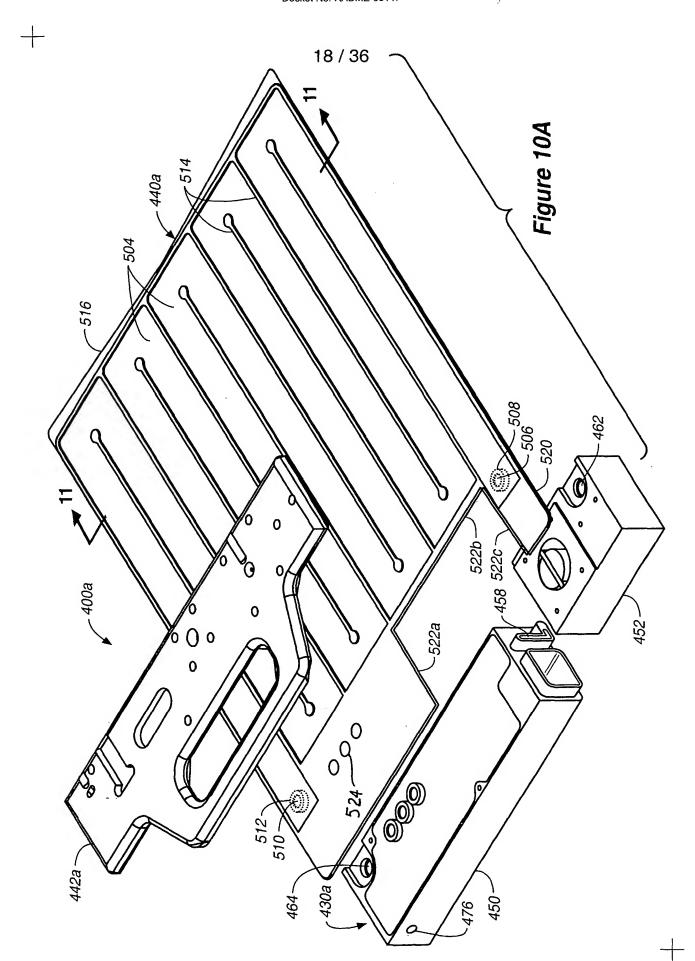


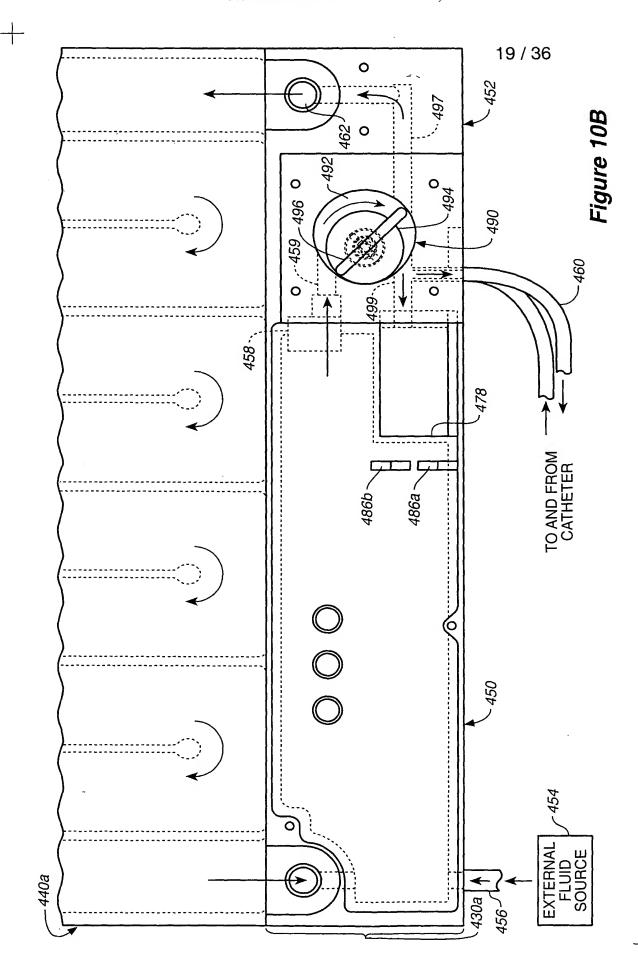




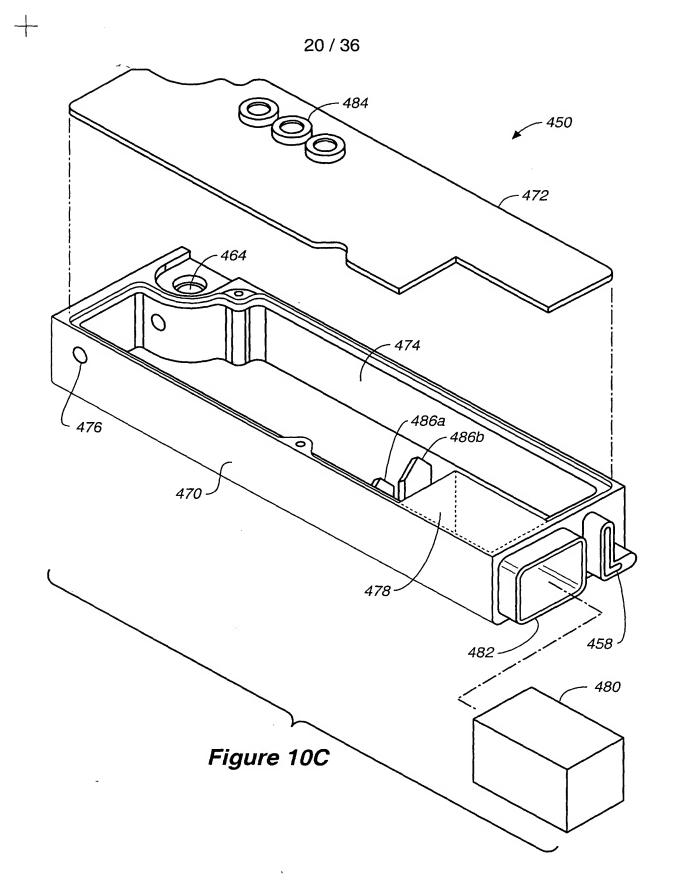


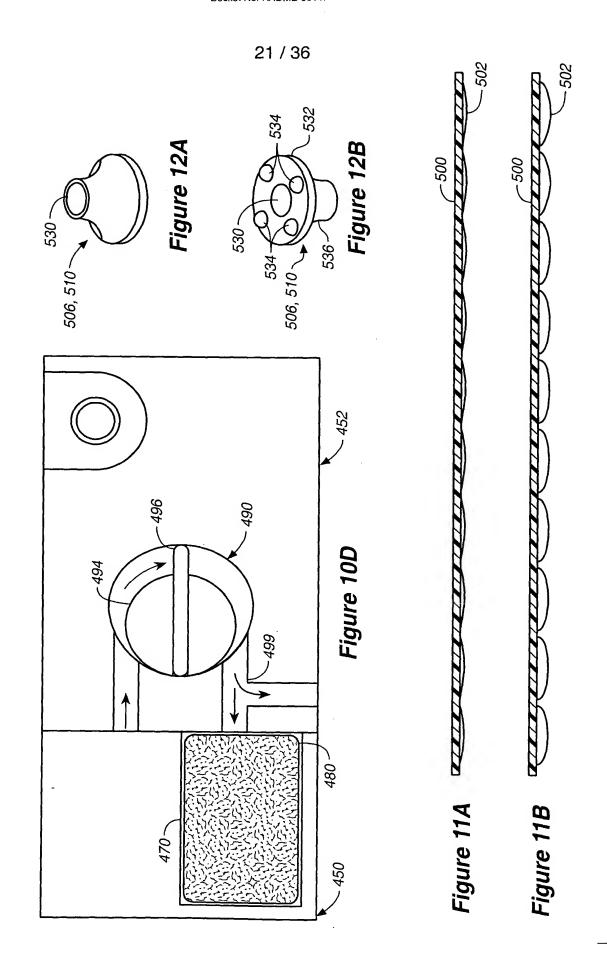

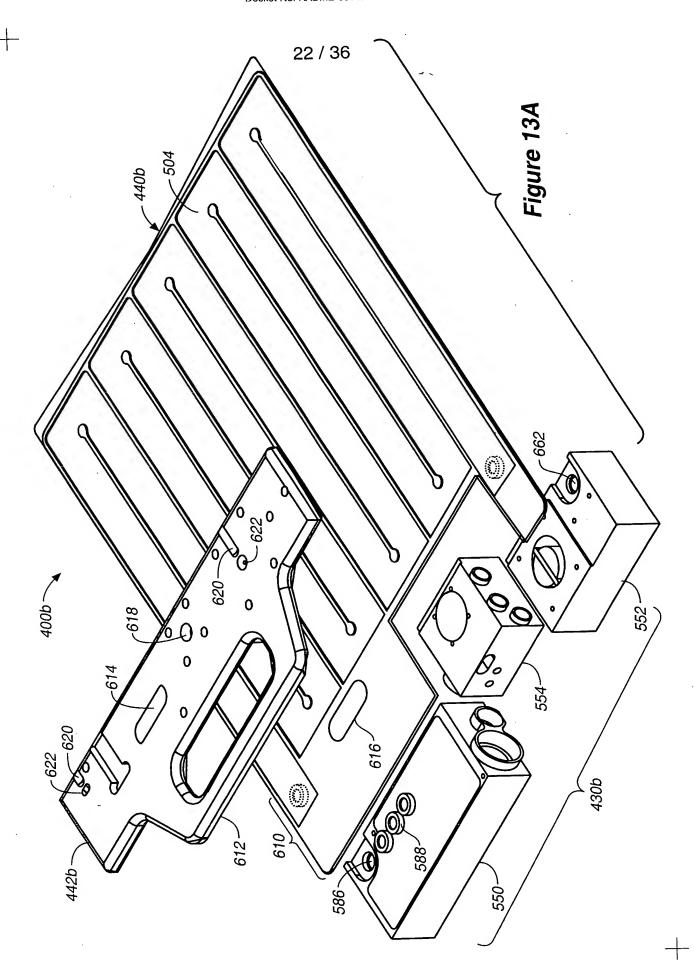

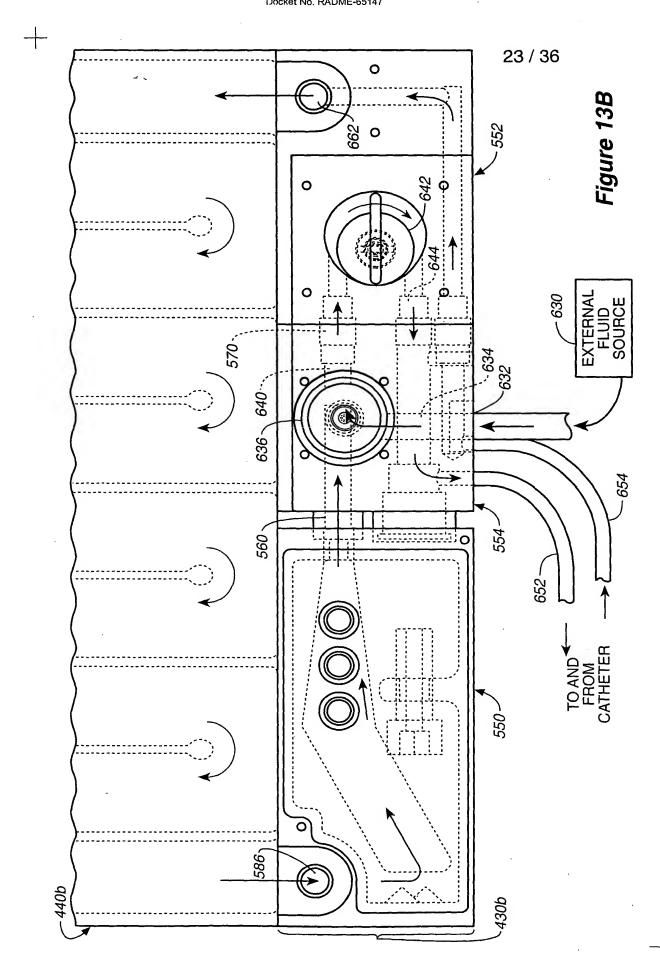

Docket No. RADME-65147

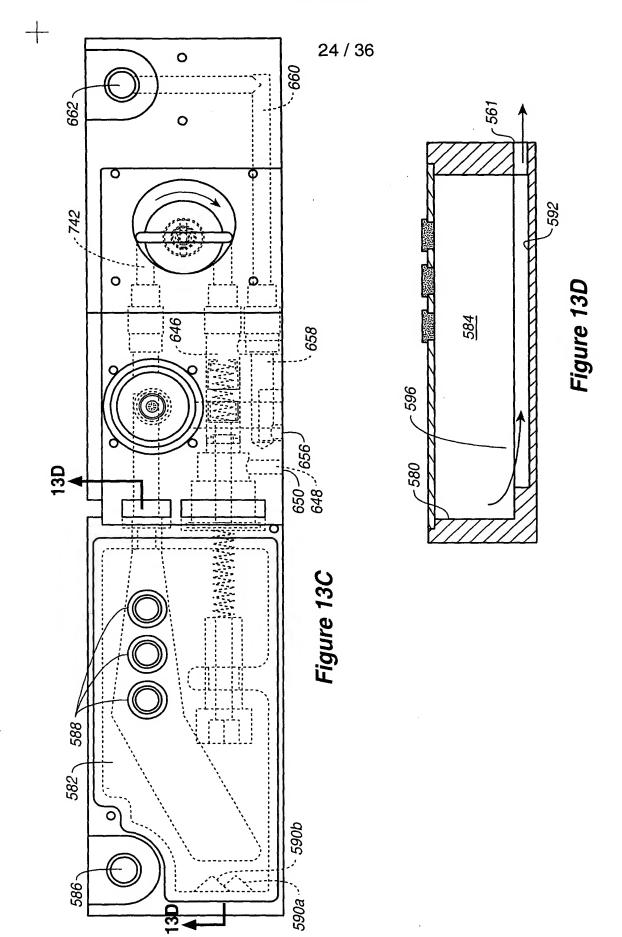

Docket No. RADMF-65147

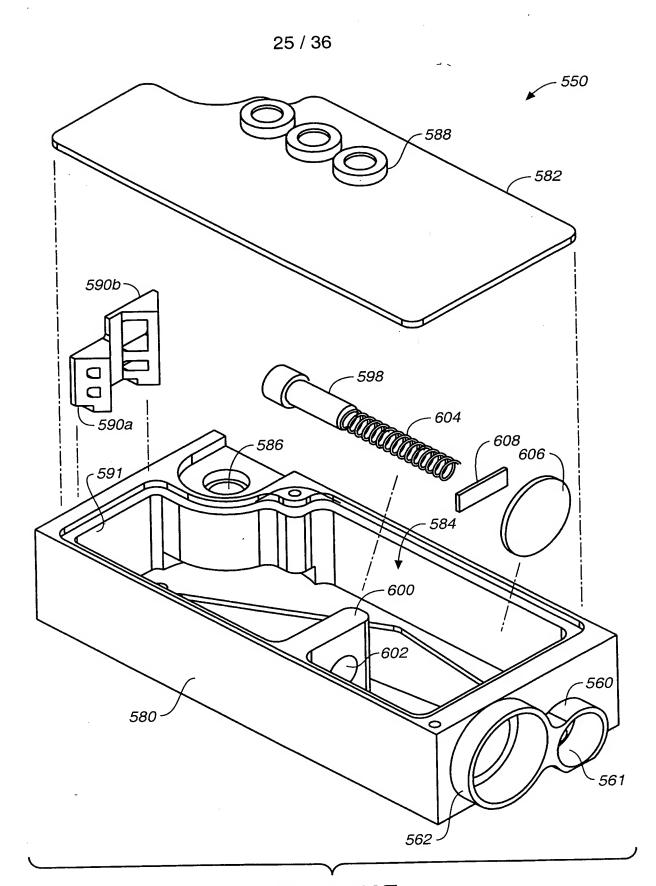
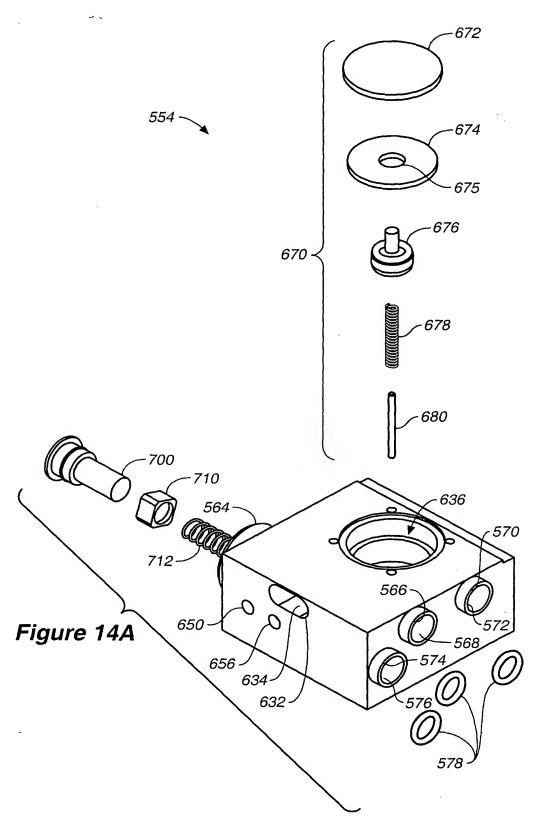
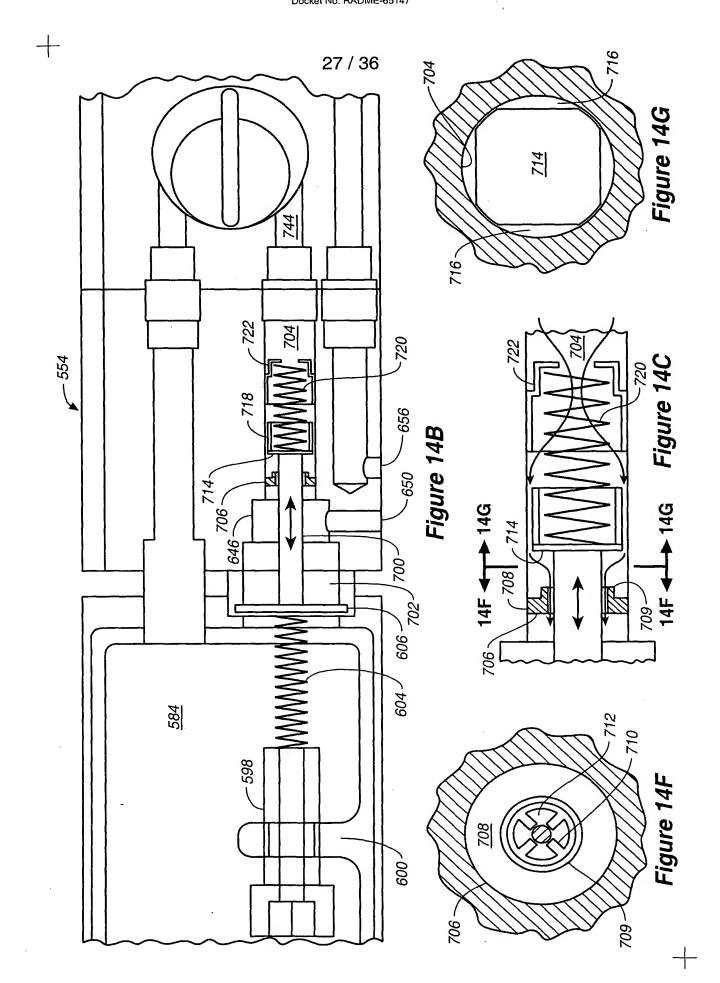
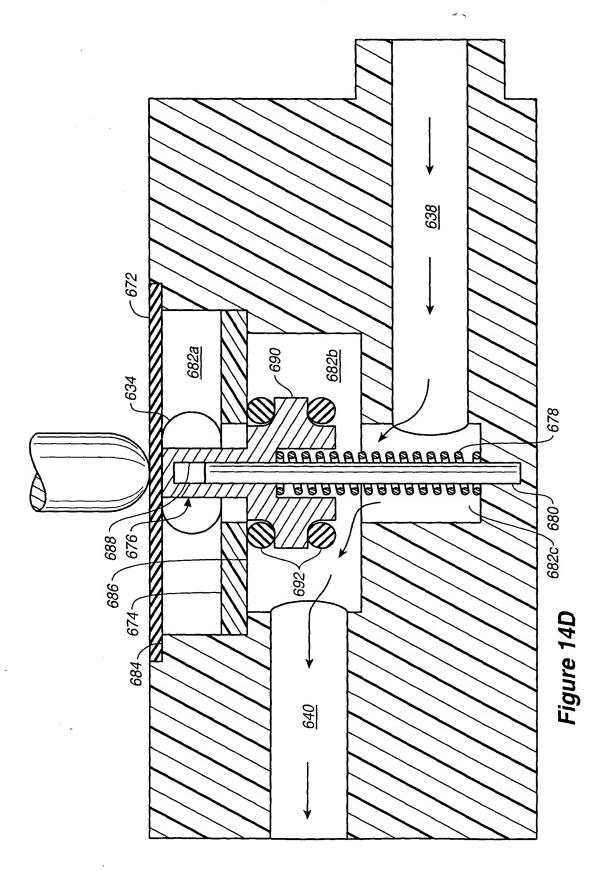


Figure 13E












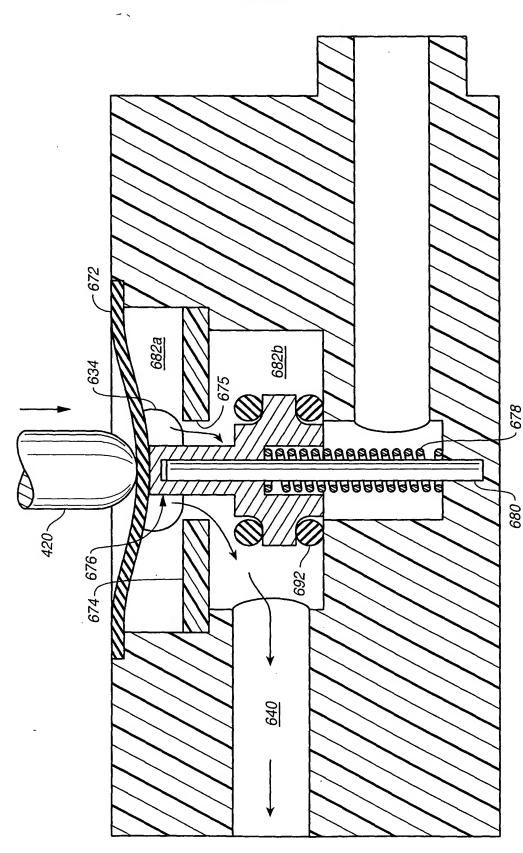


Figure 14E

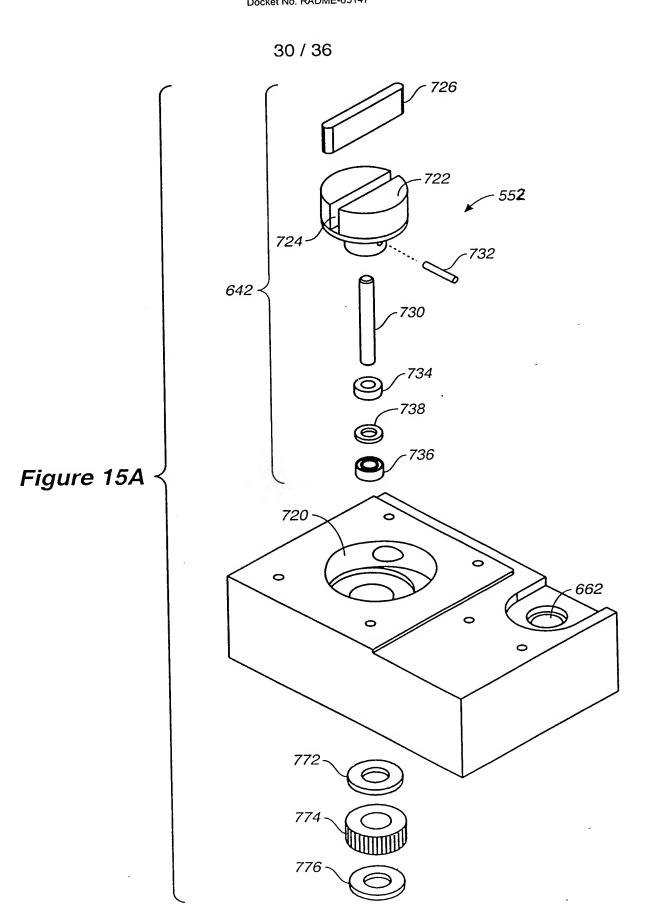

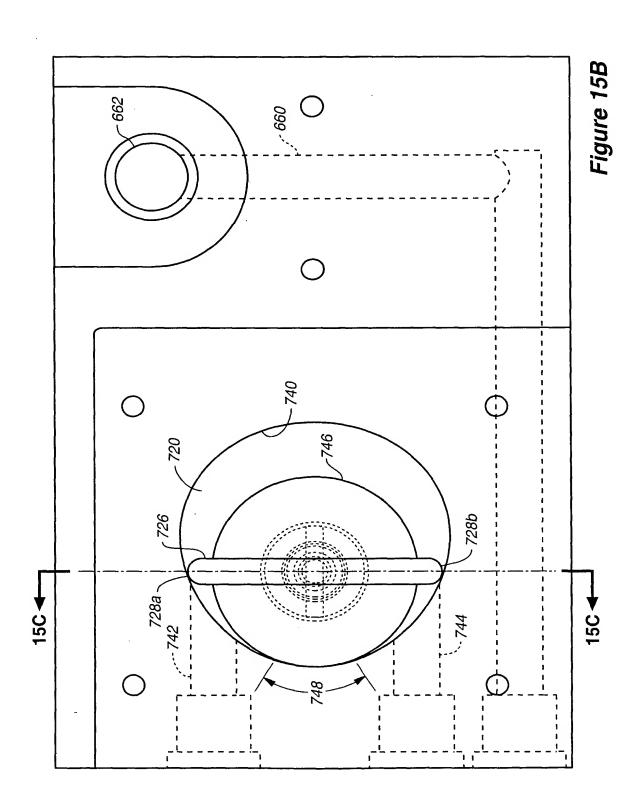

+

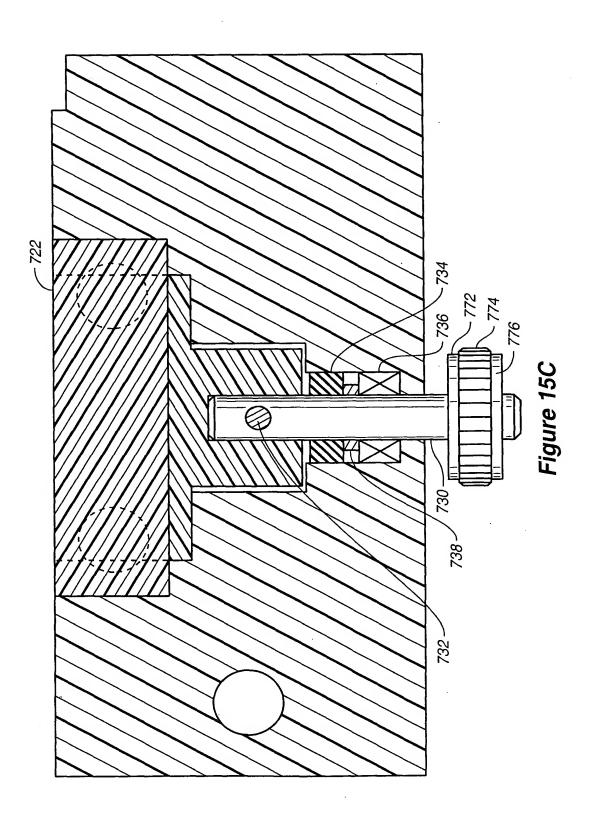

+

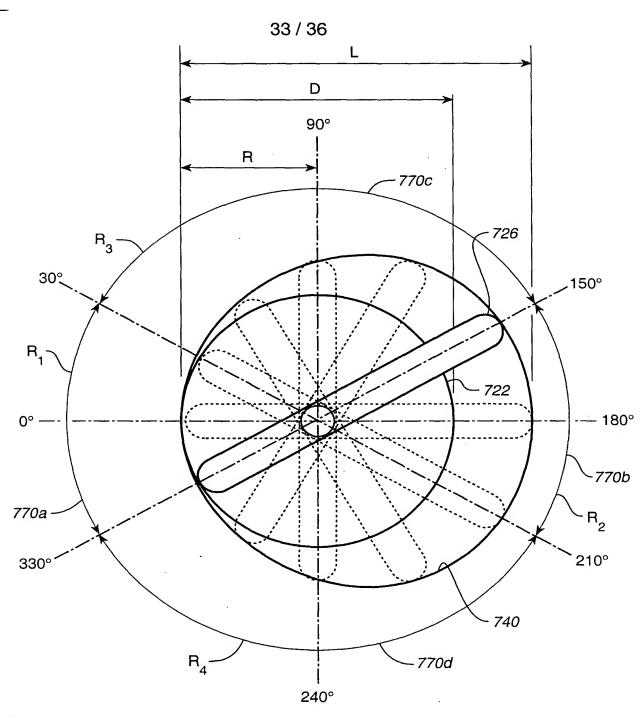


Figure 15D




Figure 16A

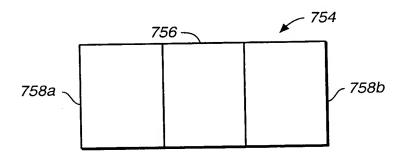


Figure 16B

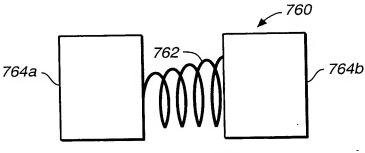


Figure 16C

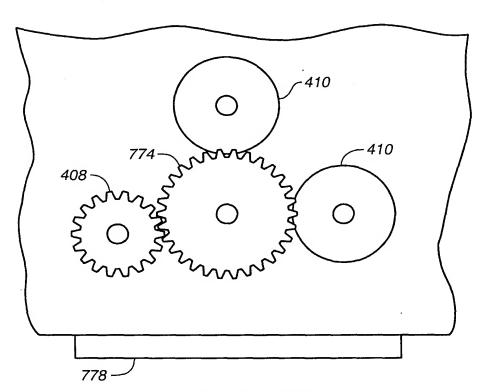


Figure 17A

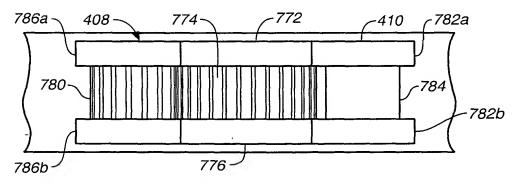


Figure 17B

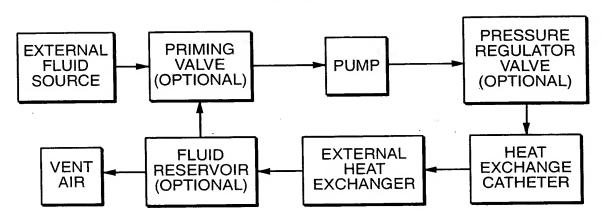


Figure 18A

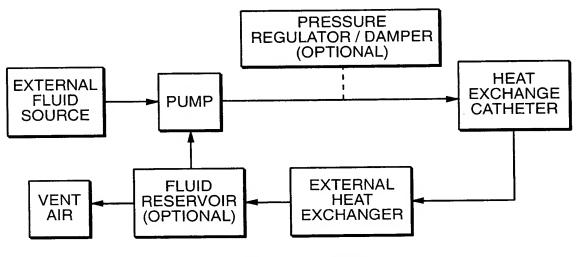


Figure 18B

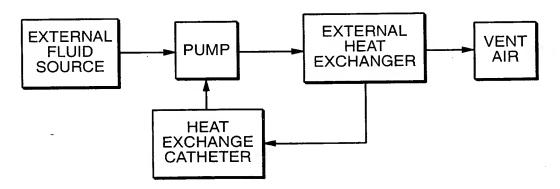


Figure 18C